


Figure 2

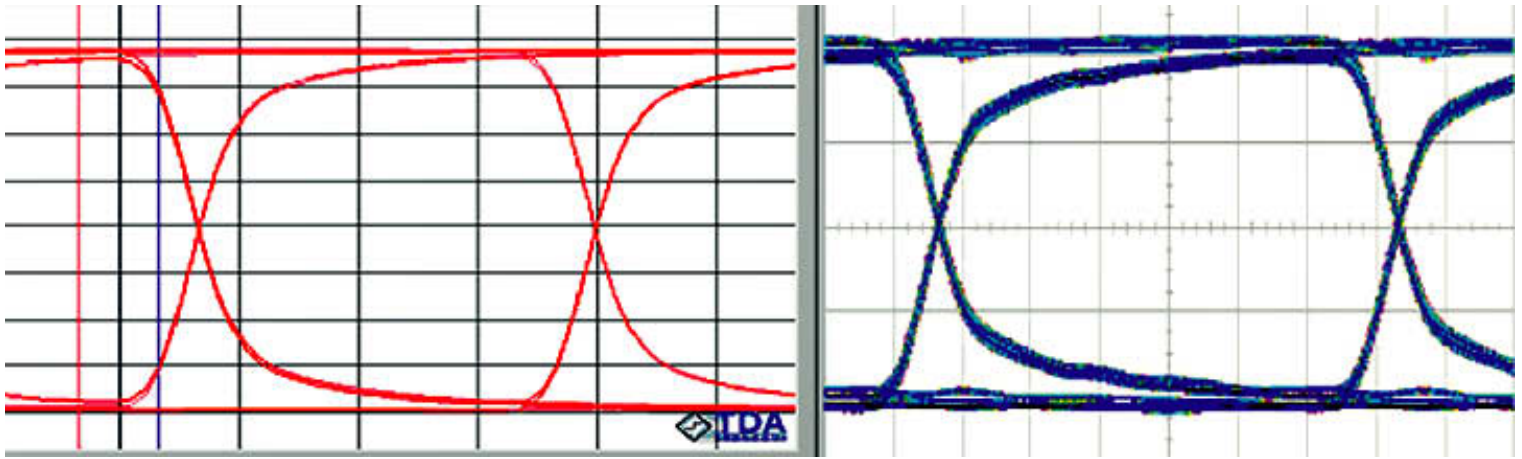

This correlation between measured and simulated eye-diagram degradation uses IConnect TDR software and TDT measurements (left) and the eye diagrams using a pattern generator (right) at a 1.5-Gbps data rate (courtesy Molex Inc).