


Figure 6

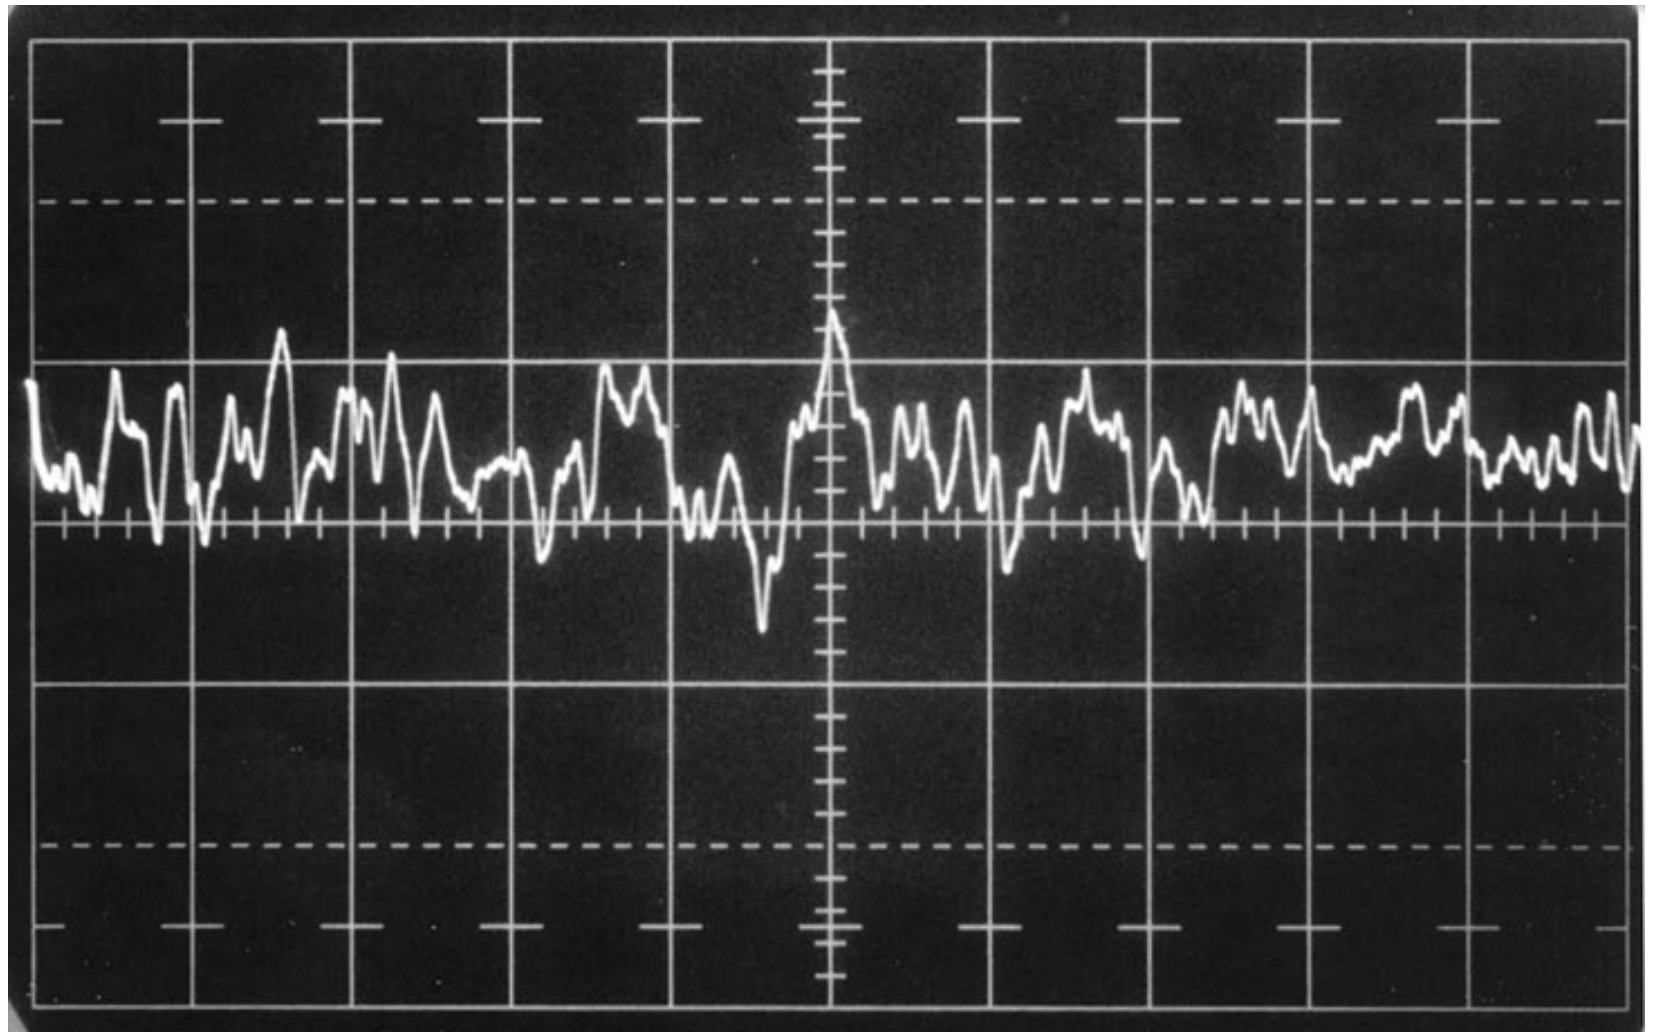

Short-term monitoring in a room environment indicates 0.001°C cooling-mode baseline stability.